

# Automatic Detection of Mass In Mammographic Images Using Dual-Tree Wavelet Transform

Heartlin Maria.H<sup>1</sup>, Evangelin Mercy Agatha.P<sup>2</sup>, Dr. P. Kavipriya<sup>3</sup>

<sup>1,2</sup>Department of ECE, Sathyabama University, Chennai – 119

<sup>3</sup>Assistant Professor, Sathyabama University Chennai - 119

-----\*\*\*-----

**ABSTRACT:** *In this paper we have proposed an improvised method in which classification of Mammographic images using neural network is involved. The proposed method involves segmentation of the Mammographic images using dual tree wavelet transform for medical analysis. The specialty of this method is that it enables the detection of cancer at early stages. This can be done by row and column segregation of the Mammographic image, which is called as bi clustering. At the end of this analysis abnormal and normal images will be sorted out. These sorted images will be then used for Computer Aided Diagnosis. The wavelet transform that is used in this method decomposes the Mammographic image to get edge details on horizontal and vertical directions, which helps in early detection of breast cancer.*


**Keywords:** Segmentation, Neural network Computer-Aided Detection (CAD), Feature extraction

## 1.INTRODUCTON

Breast cancer is a cancer that gets greater, stronger, and more complete from chest tissue. Signs of breast cancer may involve the size of an egg in the chest, a change in chest form, dimpling of the skin, liquid (or gas) coming from the pointed part, or a red scaly material put over damaged place of skin. In critical stages of the disease, there may be bone pain, swollen lymph, hard growths, shortness of breath, or yellow skin. Cancers undergoing growth from the ducts are within one's knowledge and are known as ductal carcinomas, while those undergoing growth from lobules are within one's knowledge and are known as lobular carcinomas. In addition, there are more than 18 other sub-types of Breast cancer. Some cancers undergo growth from pre-invasive lesions such as ductal carcinoma in situ. The diagnosis of Breast cancer is made likely by taking a biopsy of the about mass, bit. Once the diagnosis is made, further tests are done to come to a decision about if the cancer has put out on top beyond the chest and which treatments it may be acting in answer to. The balance of benefits against causes damage of Breast cancer going-over is open to argument. A 2013 Cochrane paper stated that it is unclear if mammographic going-over does more good or cause damage. Organization suggests going-over every 2 years in women 50 to 74 years old. The medical substances tamoxifen or raloxifene may be used in a hard work to put a stop to Breast cancer in those who are at high danger of undergoing growth it. Sorts of surgery (make, become, be) different from breast-conserving surgery to mastectomy. Chest remake may take place at the time of surgery or at a later day. In those in whom the cancer has put out on top to other parts of the body, treatments 1 are mostly directed at getting (making) better quality of living and comfort. Outcomes for Breast cancer (make, become, be) different depending on the cancer letters used for printing, size, range and degree of disease. In undergoing growth countries still living rates are poorer. Everywhere on earth, Breast cancer is the leading sort of cancer in women, accounting for 25% of all examples. In 2012 it resulted in 1.68 million 24 cases and 522,000 deaths.




**Fig(1) Normal case**

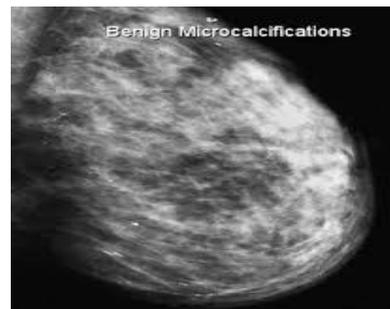

**Fig(2) Benign case**

It is not cancer and does not spread

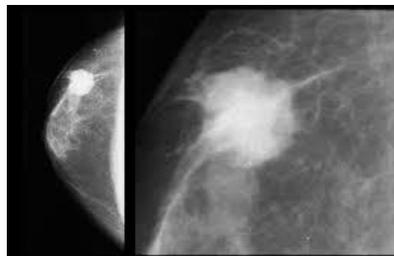

**Fig (3) malignant case**

Malignant is a type of cancer and it can spread to neighboring tissues and body parts

## 2. SURVEY ON THE PREVIOUS WORK:

Overtime there has been a lot of researches on mammogram images. Various algorithms have been used for automatic computer aided diagnosis out of which a few are as follows:

- Initially, the K-means clustering was applied for dynamically and automatically generated seed points and it determined the threshold values for each region. The region growing algorithm was used with the existing input parameters which was said to divide the mammogram into homogeneous regions based the intensity of the pixel. This method was used to automatically segment and detect the boundary of different disjoint breast tissues. Hence, using a computer-aided detection/diagnosis (CAD/CAD<sub>x</sub>) system as supplement to the radiologists' assessment has an important role. Mammographic Image Analysis Society (MIAS) database was used. The obtained results show the efficiency of this method. The disadvantage of the k-means algorithm is that the user as an input parameter must determine the number of clusters. Therefore, taking a fixed number of regions and the same regions for all images of database is irrelevant. The drawback of SRG algorithm is that the automating seed generation and dependency of output on order sorting of pixel is difficult. But in image segmentation mammograms this discontinuity is an advantage and a highlight of the kmeans algorithm.
- Being able to elucidate 3D information from stereo mammograms was an important precursor to conducting 3D digital analysis of data from this promising new modality. The problem was generally much harder than the classic stereo matching problem on visible light since almost all of the 3D structural information of interest existed as complex network of multilayered, heavily occluded curvilinear structures. Taking this problem into count, a method has been formulated where a new stereo model can minimize global energy function to densely estimate disparity on stereo mammogram images, by introducing a new singularity index as a constraint. Curvilinear structures, such as vasculature and spicules, are salient structures in the breast, and accurately positioning them in 3D was a great task. Experiments on synthetic images with known ground truth and on real stereo mammograms clearly enhances the advantages of the proposed stereo model over the canonical stereo one. Experimental results on synthetic images with known ground truth data and on real stereo mammograms show the advantages of the proposed model over the canonical model for our application. The drawback in this method is that the loss of 3D information due to the projection of the breast onto a 2D image plane. The 3D to 2D projection process results in what is commonly referred to as anatomical noise due to overlapping out of plane tissue structures. A drawback of the two baseline stereo models is that neither model is designed to promote curvilinear masses in disparity space to better preserve fine-scale curvilinear structures.
- 2D/3D registration method, which was based on biomechanical modeling of the breast, was implemented. Initially the Mammograms were segmented into fatty, glandular and tumorous tissue and then the process was carried on. For each tissue, the average sound speed and attenuation of its corresponding USCT images were calculated and noted. Tumorous tissues could be separated from fatty and glandular tissue using a fixed absolute sound speed threshold. Through combining sound speed and attenuation, the extraction of fatty tissue from glandular tissue was improvised. From sound, speed and attenuation information's that were obtained using the Mammogrammic images, required information could be obtained for diagnosis. This may benefit early breast cancer detection in future.
- A new technique for automatic extracting features of Mammogrammic images and its classification has been proposed in this paper. Hybrid processing system is used to obtain high frequency composition of mammograms and apply Radon Transform to the obtained DC transform images for extracting directional features, which in turn was fed into support vector machine for classification. This method was tested upon a hundred samples and gave accurate results.

### 3. EXISTING METHOD:

This CADe system for mammographic mass detection comprises four major stages: pre-processing, detection of suspicious mass region, feature extraction, and classification. Fig(4) shows an overview of the proposed mass detection scheme, and the following section presents each component in detail

#### 3.1 Screenshot of the output


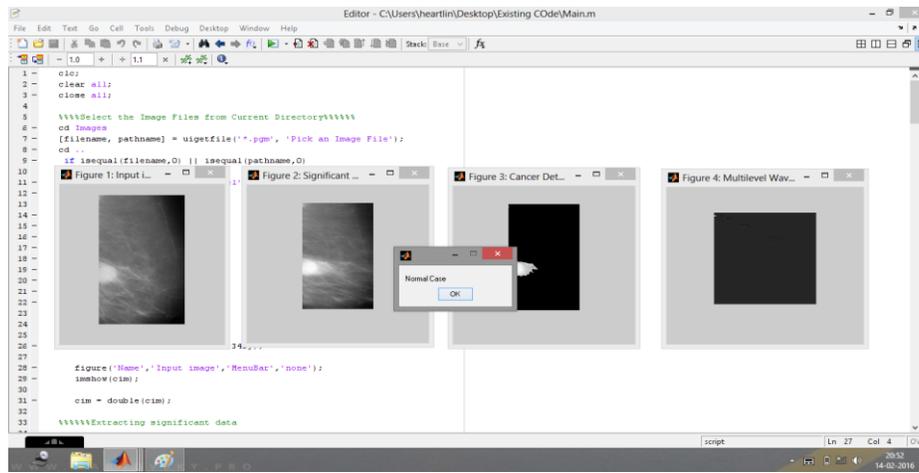


Fig (4)

#### 3.2 Discussion and conclusion

This study presents an automatic CADe system for mammographic mass detection that uses complex texture features. This system first pre-processes a mammogram to acquire the breast region and suppress the effects of blood vessels, glandular tissues, and noises using morphological filters. This study proposes two feature extraction modules combining co-occurrence matrix texture features and optical density features. One of the extraction methods, which is a combination of GLCM features and optical density features, describes both the gray-level characteristics of local textures and photometric discrete textures based on the global optical density. The other module, which combines ODCM features with optical density features, is similar to the former, but characterizes local textures in an optical density image instead of the gray-level image. Further, the optical density image that enlarges the difference near the special target brightness is proposed. The difference of gray level near the normal tissue intensity is particularly concerned, because the margin brightness of a mass is always close to the normal tissue. The optical density image enhances the difference of gray level based on the normal tissue intensity to strengthen the description of the suspicious area shape for feature extraction in CADe system. Other image enhancement algorithms promote contrast based on overall gray scale distribution that is different from the optical density image. The experiments in this study prove that the proposed scheme with LDA achieves satisfactory detection sensitivity with an acceptable FP rate for both two feature extraction methods. Moreover, the deep analysis of different breast density rating reveal that the GLCM-optical density features manifest the better performance in the lower density mammogram, and ODCM-optical density features express the better performance in the higher density mammogram. The breast density is based on how much the breast is made up of fatty tissue versus how much is made up of fibrous and glandular.

#### 4. PROPOSED METHOD

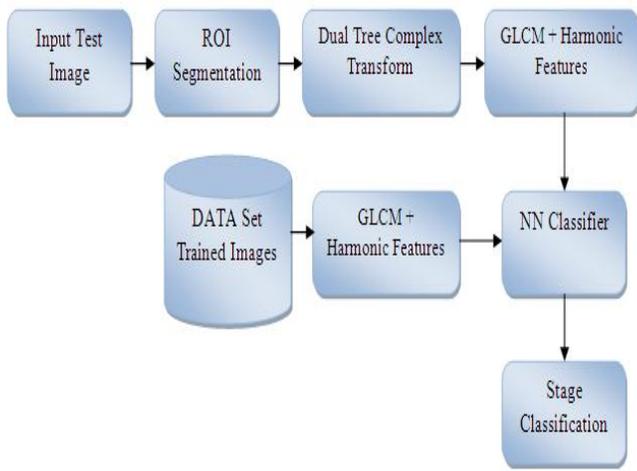

#### Gray Level Cooccurrence Features

- **Energy :**  $E = \sum_x \sum_y p(x, y)^2$   $p(x, y)$  is the GLCM
- **Contrast :**  $Contrast = I = \sum_x \sum_y (x-y)^2 p(x, y)$
- **Entropy :**  $S = -\sum_x \sum_y p(x, y) \log p(x, y)$
- **Correlation Coefficient :**  

$$\frac{\sum_x \sum_y (x - \mu_x)(y - \mu_y) p(x, y)}{\sigma_x \sigma_y}$$

Fig (5) shows the block diagram of the proposed method

#### 4.2 Explanation

##### Dual-Tree wavelet transform


Dual-tree discrete wavelet transform (DWT) provides advantages over the critically sampled DWT for signal and image processing. The dual-tree DWT is implemented as two separate two-channel filter banks. To gain the advantages described in this example, you cannot arbitrarily choose the scaling and wavelet filters used in the two tree.

#### 4.3 COMPARISON OF ACCURACY AND SPECIFICITY

S.No	Parameter	Existing Method (Complex Wavelet Transform)	Proposed Method (Dual Tree Wavelet Transform)
1	Sensitivity	100%	100%
2	Specificity	80%	90%
3	Accuracy	92.3077%	94.7368%

Table-1

#### 4.4 GUI output screenshot

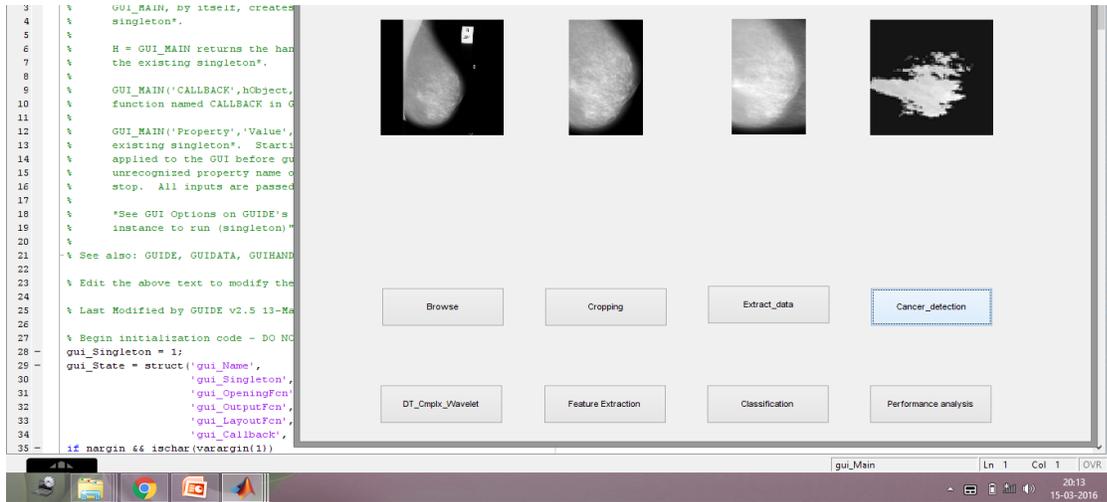

Fig(6)

#### 4.5 Screenshot of accuracy, sensitivity and specificity of proposed method



Fig(7)

